

Mycoplasma Testing Results

(MycoStrip – Invivo Lot: 10619-4503)

Date: 10th April 2023


<u>Location</u>	<u>Band (C/and or T)</u>	<u>Results</u>	<u>Pass/Fail</u>
Carboy 1	C	Negative	Pass
Stream	C	Negative	Pass
Sheath Tank 1	C	Negative	Pass
Sheath Tank 2	C	Negative	Pass
Sheath Tank 3	C	Negative	Pass
Sheath Tank 4	C	Negative	Pass
Sheath Tank 5	C	Negative	Pass
Positive Control	C and T	Positive	Pass

Interpretation:

C Band: Mycoplasma Not Detected

T Band: Mycoplasma Detected

Results:

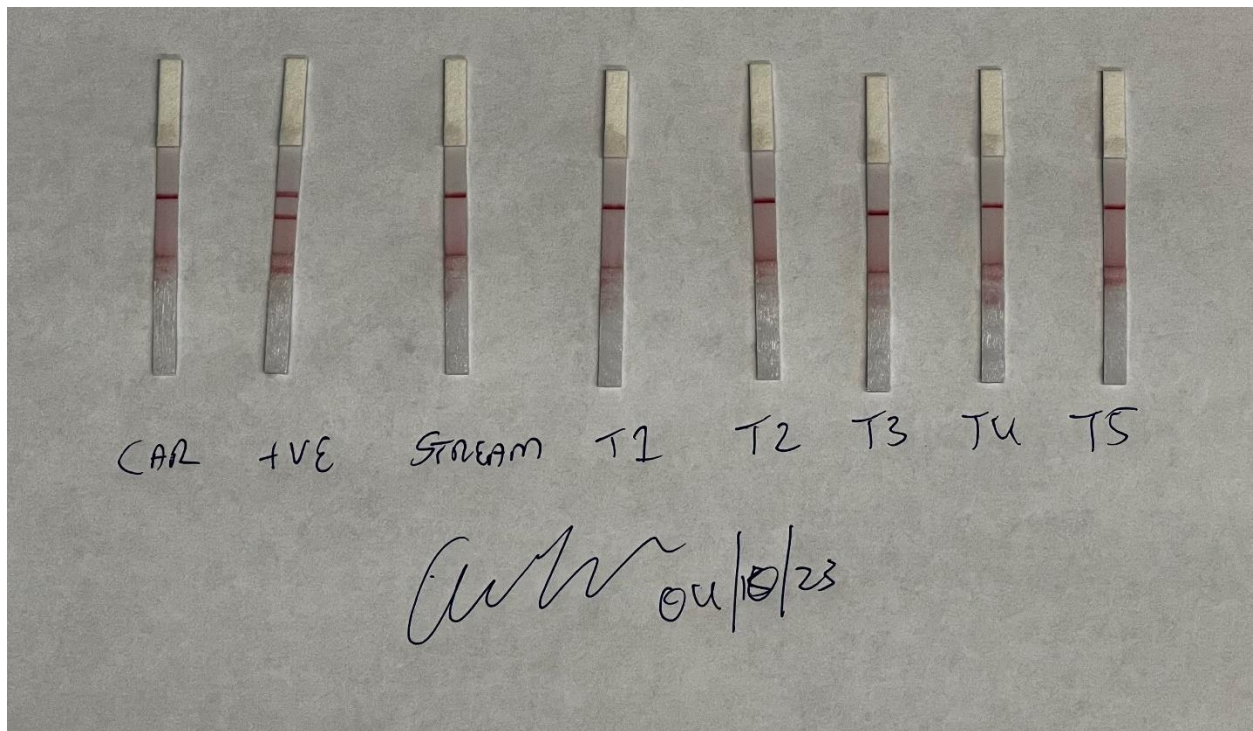

Remarks: New sheath tanks purchased and now autoclaved separately from PBS. Sterile, endotoxin and mycoplasma tested PBS purchased from Lifecycle. PBS transferred in Class II biosafety cabinet into sterile sheath tanks.