

**Mycoplasma Testing Results**

(MycoStrip – Invivo Lot: 10619-4503)

Date: 10<sup>th</sup> August 2023


<u>Location</u>	<u>Band (C/and or T)</u>	<u>Results</u>	<u>Pass/Fail</u>
Carboy 1	C	Negative	Pass
Stream	C	Negative	Pass
Sheath Tank 1	C	Negative	Pass
Sheath Tank 2	C	Negative	Pass
Sheath Tank 3	C	Negative	Pass
Sheath Tank 4	C	Negative	Pass
Sheath Tank 5	C	Negative	Pass
CS Sheath Tank 1	C	Negative	Pass
CS Sheath Tank 2	C	Negative	Pass
Positive Control	C and T	Positive	Pass

**Interpretation:**

**C Band: Mycoplasma Not Detected**

**T Band: Mycoplasma Detected**

**Results:**

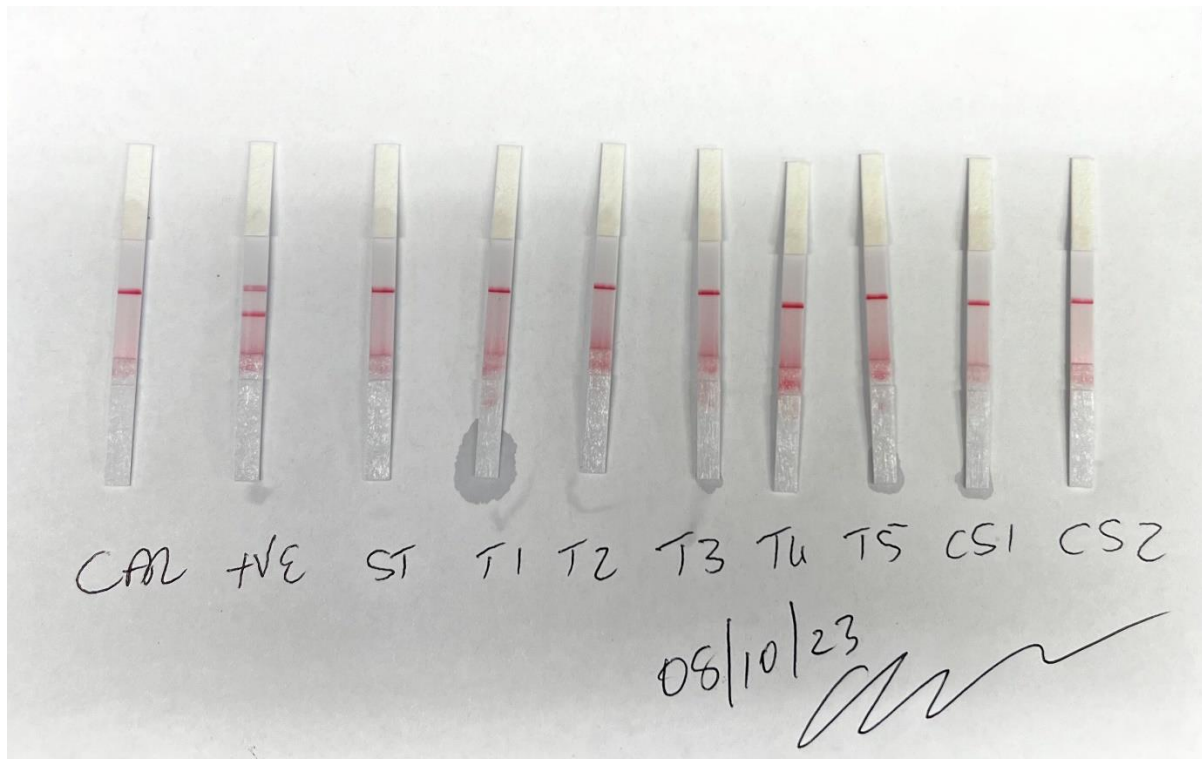

**Remarks:** New sheath tanks purchased and now autoclaved separately from PBS. Sterile, endotoxin and mycoplasma tested PBS purchased from Lifecycle. PBS transferred in Class II biosafety cabinet into sterile sheath tanks.