

**ACCUTECH Inc.**

1219 Hardin Bridge Rd SW  
 Euharlee, GA 30145  
 victoria@accutechcalibrations.com  
 404-861-8605

**INVOICE / WORKSHEET**

Building <u>HSRB - Emory</u>	INVOICE # <u>0731242C</u>
Address <u>Hwy 980</u>	PO/Acct.#
Client Name <u>CTDC</u>	Phone # <u>727-2343</u>
Service Date <u>July 31, 2024</u>	Page Number <u>1</u> of <u>2</u>
Lab/ Room # <u>E-204</u>	Email:

**Calibration Record**

		SAMPLE DRAWS					FINAL DRAWS				
	PIPETTE #	Volume	LOW	MID	HIGH	Pass/Fail	SERVICE REQUIRED	LOW	MID	HIGH	Cost
1	SU19322	100	Out of Tolerance			Fail	Calibrate	199.1	50.01	100.06	25 <sup>00</sup>
2	OU14246	100	Out of Tolerance			Fail	Calibrate	19.91	50.01	100.09	25 <sup>00</sup>
3	SU11623	20	5.00	10.01	20.03	Pass	OK				0
4	L1426707	1000	Out of Tolerance			Fail	Calibrate	202.01	500.02	997.85	25 <sup>00</sup>
5	L14295597	200	50.01	100.10	200.22	Pass	OK				0
6	L14355057	100	20.10	50.07	100.01	Pass	OK				0
7	L14297437	100	20.21	50.11	100.03	Pass	OK				0
8	L14343237	20	5.10	9.96	20.01	Pass	OK				0
9	L14340897	2	0.50	1.00	2.01	Pass	OK				0
10	OU17090	<sup>12-24</sup> 300	Out of Tolerance			Fail	Calibrate	49.59	150.01	300.07	35 <sup>00</sup>
11	RU12929	1000	Out of Tolerance			Fail	Calibrate	200.01	499.89	997.77	25 <sup>00</sup>
12	SU11505	1000	Out of Tolerance			Fail	Calibrate	198.91	499.67	1001.80	25 <sup>00</sup>
13	SU11507	1000	Out of Tolerance			Fail	Calibrate	198.94	500.01	996.68	25 <sup>00</sup>
14	QU37735	1000	Out of Tolerance			Fail	Calibrate	198.85	499.51	1004.48	25 <sup>00</sup>
15	SU11508	1000	Out of Tolerance			Fail	Calibrate	198.74	500.11	1001.20	25 <sup>00</sup>
16	SU01550	1000	Out of Tolerance			Fail	Calibrate	198.33	499.79	1001.29	25 <sup>00</sup>
17	RU12924	1000	Out of Tolerance			Fail	Calibrate	198.99	497.76	1002.71	25 <sup>00</sup>
18	RU04927	300	Out of Tolerance			Fail	Calibrate	49.99	150.04	300.13	25 <sup>00</sup>
19	SU11679	300	Out of Tolerance			Fail	Calibrate	49.71	150.01	300.13	25 <sup>00</sup>
20	SU11675	300	Out of Tolerance			Fail	Calibrate	49.23	149.91	300.80	25 <sup>00</sup>

Page Total \$ 360

Parts Replaced \_\_\_\_\_ @ \$ \_\_\_\_\_ Each  
 \_\_\_\_\_ @ \$ \_\_\_\_\_ Each  
 \_\_\_\_\_ @ \$ \_\_\_\_\_ Each  
 \_\_\_\_\_ @ \$ \_\_\_\_\_ Each



TOTAL AMOUNT DUE \$ See Page 2

Technician Zachary Cleaver

Customer Signature \_\_\_\_\_

Balance 11909521 Nist Wt. 200g Water 22 C. Z-Factor 1.0022

#Calibrated 14 Next Calibration Due Date Feb 1, 2025

**ACCUTECH Inc.**

**INVOICE / WORKSHEET**

1219 Hardin Bridge Rd SW  
 Euaharlee, GA 30145  
 victoria@accutechcalibrations.com  
 404-861-8605

Building <u>HSRB - Emory</u>	INVOICE # <u>0731242C</u>
Address <u>Haygood</u>	PO/Acct.# _____
Client Name <u>CTDC</u>	Phone # <u>727-2343</u>
Service Date <u>July 31, 2024</u>	Page Number <u>2</u> of <u>2</u>
Lab/ Room # <u>E-264</u>	Email: _____

**Calibration Record**


**SAMPLE DRAWS**

**FINAL DRAWS**

	PIPETTE #	Volume	SAMPLE DRAWS			Pass/Fail	SERVICE REQUIRED	FINAL DRAWS			Cost
			LOW	MID	HIGH			LOW	MID	HIGH	
1	✓ Ru05037	300	Out of Tolerance			Fail	Calibrate	49.43	150.03	301.03	25 <sup>00</sup>
2	Ru37793	200	Out of Tolerance			Fail	Calibrate	49.94	100.01	200.37	25 <sup>00</sup>
3	✓ Ou17222	200	Out of Tolerance			Pass	<del>Calibrate</del>	49.89	100.07	200.50	∅
4	Ru12914	100	Out of Tolerance			Fail	Calibrate	19.88	49.99	100.16	25 <sup>00</sup>
5	Ru12909	100	Out of Tolerance			Fail	Calibrate	19.87	50.01	100.10	25 <sup>00</sup>
6	Su20765	100	Out of Tolerance			Fail	Calibrate	19.87	49.98	100.09	25 <sup>00</sup>
7	✓ Su11612	20	Out of Tolerance			Fail	Calibrate	5.07	10.06	20.07	25 <sup>00</sup>
8	✓ Ru10797	10	Out of Tolerance			Fail	Calibrate	1.95	4.99	10.08	25 <sup>00</sup>
9	Ru12899	10	Out of Tolerance			Fail	Calibrate	2.01	5.03	10.07	25 <sup>00</sup>
10	Ou17272	2	0.50	1.00	2.01	Pass	OK				∅
11											
12											
13											
14											
15											
16											
17											
18											
19											
20											

Page Total \$ 200

Parts Replaced \_\_\_\_\_ @ \$ \_\_\_\_\_ Each  
 \_\_\_\_\_ @ \$ \_\_\_\_\_ Each  
 \_\_\_\_\_ @ \$ \_\_\_\_\_ Each  
 \_\_\_\_\_ @ \$ \_\_\_\_\_ Each

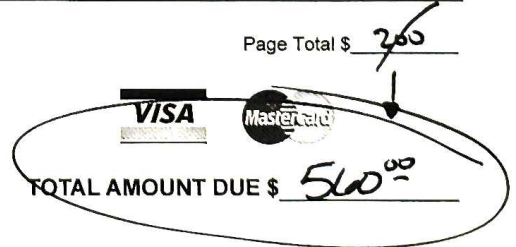

Technician Zachary Cleaver

Customer Signature \_\_\_\_\_

Balance 11902521 Nist Wt. 2065 Water 22 C. Z-Factor 1.0022

#Calibrated 8 Next Calibration Due Date Feb 1, 2025

22 of 30 calibrated